MIDMARK® Installation Instructions

9A155001 Printer Kit Installation For M9 & M11 Sterilizers

KIT COMPONENTS

Part Number	Description	Qty.
9A155001	Printer Kit	1
003-0826-00	Installation Instructions	1

REQUIRED TOOLS

Phillips Screwdriver

IMPORTANT INSTRUCTIONS

Provides a means to add a printer to the Sterilizer in order to print out pertinent data during the sterilization process.

NOTE

Applies To Model M9A (AUSTRALIAN)

Newer M9A units come from factory with printer harness already installed. Due to this fact, it will not be necessary to complete some of the steps that pertain to installation of the harness. The printer harness that comes with the printer kit can be discarded.

WARNING

Always disconnect power cord from outlet before removing any sterilizer covers/panels or making any repairs to prevent possibility of electrical shock and allow unit to cool. Failure to comply could result in personal injury.

INSTALLATION (1)

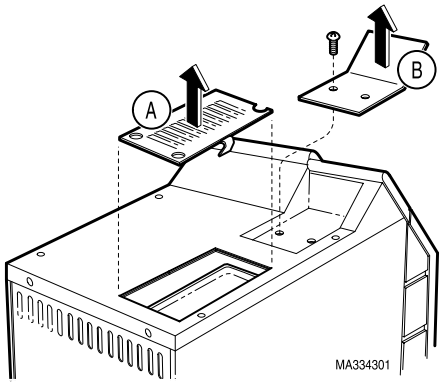

A. Unplug Sterilizer from wall outlet and allow unit to cool, then remove top inspection cover.

NOTE

After removal, place printer cover plate and two screws in storage in case printer is removed in the future and these parts are needed again.

B. Remove two screws and printer cover plate.

INSTALLATION (2)

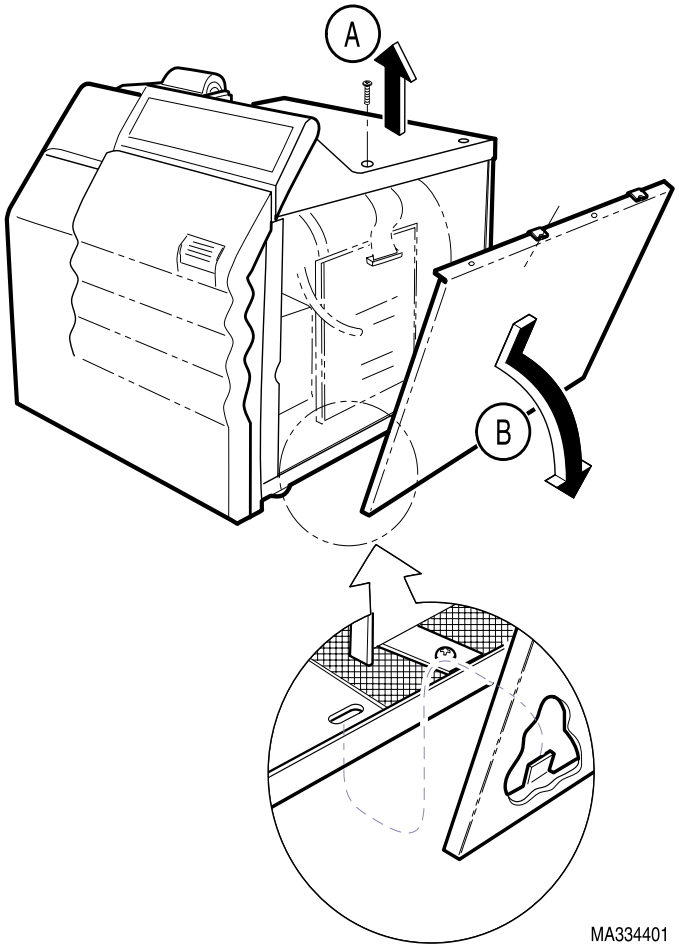

A. Remove two screws from top cover

B. Pull outward and down on on top edge of right side panel and remove panel.

© Midmark Corporation - 1999

INSTALLATION (3)

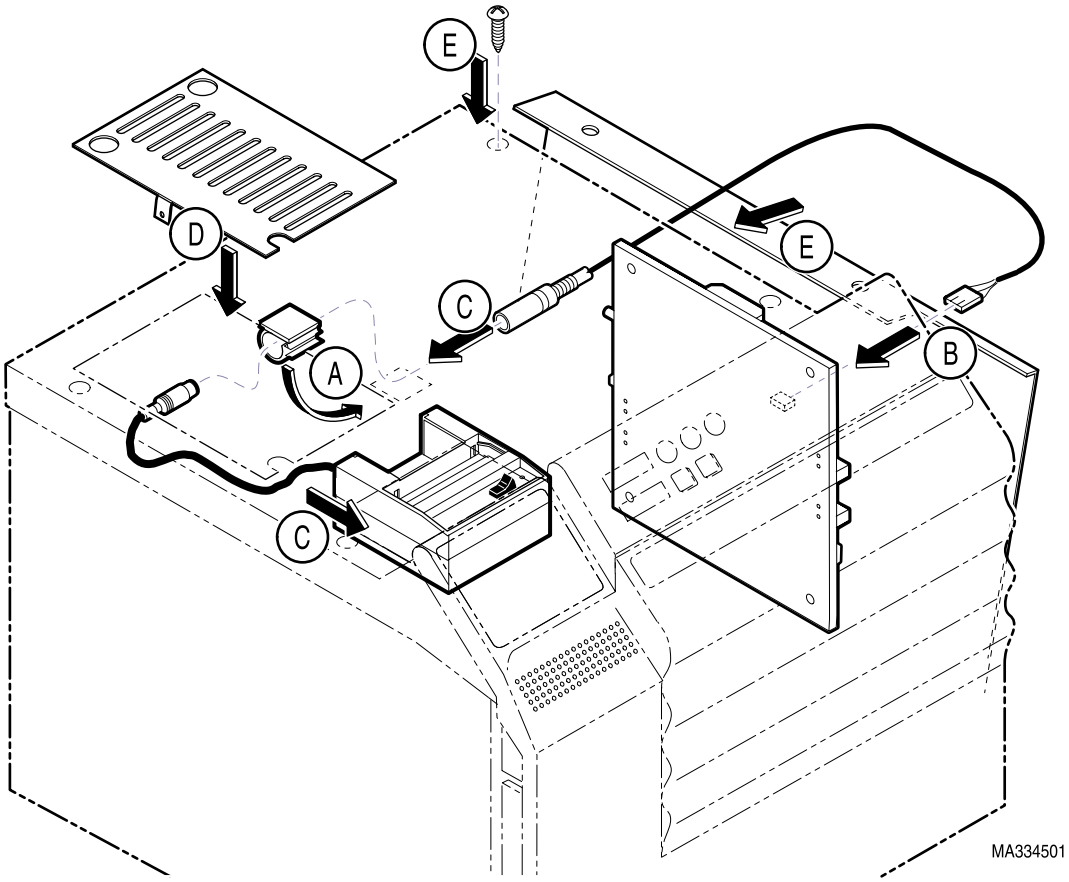

NOTE

Harness clip must be installed on inside surface of top cover at the front, right corner of the inspection opening, , that *does not* contain the conductive coating.

A. Remove protective paper from adhesive of harness clip and press in position on inside of top cover.

B. Insert rectangular plug onto J3 pin connector (marked Printer Cable) on the main P.C. board.

EQUIPMENT ALERT

Assure printer harness is routed from p.c. board, inside covers, and through harness clip to prevent it from contacting the hot pressure relief valve that could harm cable.

C. Place printer in recess area of top cover and connect printer harness plug into printer.

D. Place top inspection cover in position assuring printer cable is routed through u-shaped cutout in cover.

E. Install side panel and plug unit into wall outlet and check operation using the instructions in the Installation / Operation Manual for the Sterilizer.

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

© Midmark Corporation - 1999